



09/759387

COFC

PATENT
15-CT-5419

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Patent No.: 6,873,678 B2

Issued: March 29, 2005

Inventors: David M. Hoffman

Assignee: GE Medical Systems Global
Technology Company, LLC

For: METHODS AND APPARATUS FOR
COMPUTED TOMOGRAPHIC CARDIAC OR
ORGAN IMAGING

Certificate
JUL 08 2005
of Correction

CERTIFICATE OF MAILING

I certify that this correspondence is being deposited with the United States Postal Service as first class mail in an envelope addressed to: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450, on June 29, 2005.

Robert B. Reeser, III
Reg. No. 45,548

Hon. Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450.

REQUEST FOR CERTIFICATE OF CORRECTION OF
PATENT UNDER 37 C.F.R. 1.322(a)

Sir:

Attached, in duplicate, is Form PTO/SB/44 with one copy being suitable for printing.

In Claim 3, column 8, line 33, after "x-direction" delete "and" and insert therefor --
transverse to --.

JUL - 8 2005


The correction is not due to any error by applicants and no fee is due.

The Assignment for this patent is recorded on Reel 011417/ Frame 0250.

Date:

Sept 29, 2005

Respectfully submitted,

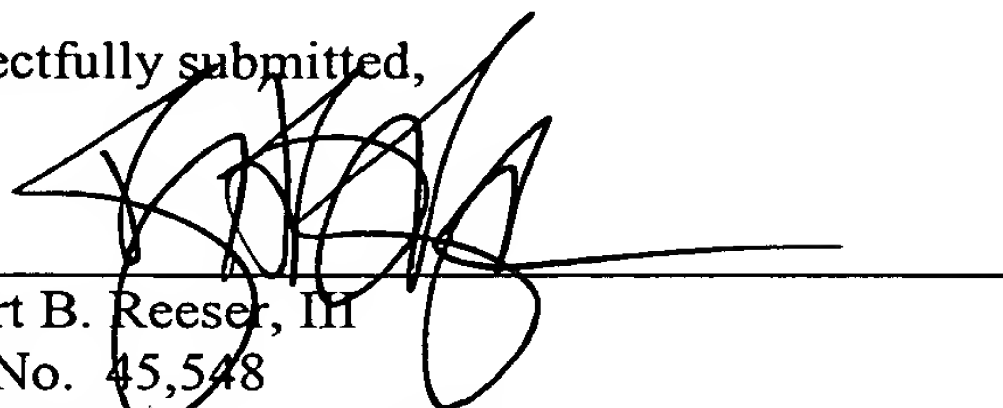

Robert B. Reeser, III

Reg. No. 45,548

ARMSTRONG TEASDALE LLP

One Metropolitan Square, Suite 2600

St. Louis, Missouri 63102-2740

(314) 621-5070

UNITED STATES PATENT AND TRADEMARK OFFICE CERTIFICATE OF CORRECTION

PATENT NO : 6,873,678 B2
DATED : March 29, 2005
INVENTORS(S) : David M. Hoffman

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In Claim 3, column 8, line 33, after "x-direction" delete "and" and insert therefor -- transverse to --.


MAILING ADDRESS OF SENDER:
Robert B. Reeser, III
Armstrong Teasdale LLP
One Metropolitan Sq., Suite 2600
St. Louis, MO 63102

PATENT NO. 6,873,678 B2

No. of additional copies

This collection of information is required by 37 CFR 1.322, 1.323, and 1.324. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 1.0 hour to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Attention Certificate of Corrections Branch, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

JUL - 8 2005

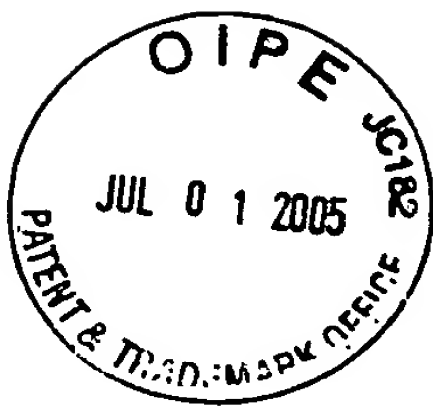

PATENT
15-CT-5419

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Patent No.: 6,873,678 B2

Issued: March 29, 2005

Inventors: David M. Hoffman

Assignee: GE Medical Systems Global
Technology Company, LLC

For: METHODS AND APPARATUS FOR
COMPUTED TOMOGRAPHIC CARDIAC OR
ORGAN IMAGING

CERTIFICATE OF MAILING

I certify that this correspondence is being deposited with the United States Postal Service as first class mail in an envelope addressed to: Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450, on June 29, 2005.

Robert B. Reeser, III
Reg. No. 45,548

Hon. Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450.

REQUEST FOR CERTIFICATE OF CORRECTION OF
PATENT UNDER 37 C.F.R. 1.322(a)

Sir:

Attached, in duplicate, is Form PTO/SB/44 with one copy being suitable for printing.

In Claim 3, column 8, line 33, after "x-direction" delete "and" and insert therefor --
transverse to --.


The correction is not due to any error by applicants and no fee is due.

The Assignment for this patent is recorded on Reel 011417/ Frame 0250.

Date:

Sept 29, 2005

Respectfully submitted,

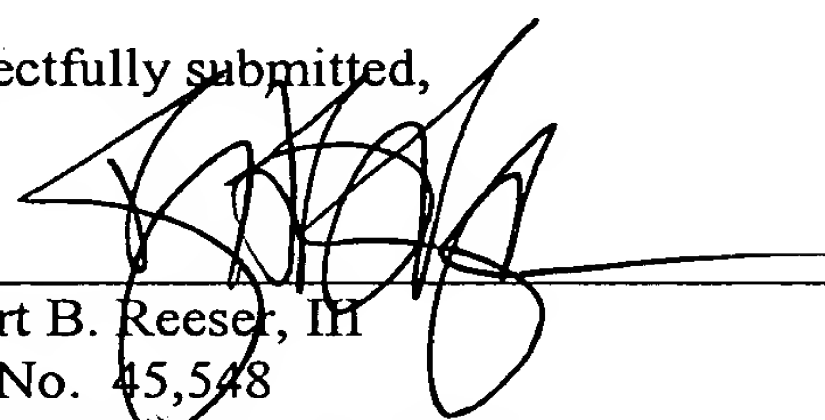

Robert B. Reeser, III
Reg. No. 45,548
ARMSTRONG TEASDALE LLP
One Metropolitan Square, Suite 2600
St. Louis, Missouri 63102-2740
(314) 621-5070

UNITED STATES PATENT AND TRADEMARK OFFICE CERTIFICATE OF CORRECTION

PATENT NO : 6,873,678 B2
DATED : March 29, 2005
INVENTORS(S) : David M. Hoffman

It is certified that error appears in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

In Claim 3, column 8, line 33, after "x-direction" delete "and" and insert therefor -- transverse to --.

MAILING ADDRESS OF SENDER:
Robert B. Reeser, III
Armstrong Teasdale LLP
One Metropolitan Sq., Suite 2600
St. Louis, MO 63102

PATENT NO. 6,873,678 B2

No. of additional copies

This collection of information is required by 37 CFR 1.322, 1.323, and 1.324. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 1.0 hour to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. SEND TO: Attention Certificate of Corrections Branch, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.

JUL - 8 2005

JUL - 8 2005